

corpuls cpr Quick Guide Scoopboard

Information on corpuls cpr

- The **corpuls cpr** is a device for mechanical chest compressions within the framework of cardiopulmonary resuscitation.
- This is a basic guide for use and procedures adopted by your service may differ slightly.

Preparing the corpuls cpr for use

 The corpuls cpr device will be stored in its dedicated carry bag and on charge.



2. Remove the Scoopboard from the front pocket of the bag.




- 3. The socket can only be positioned by the patient's right shoulder.
- 4. Log roll or shoulder lift the patient to insert the Scoopboard, ensuring interruptions to manual cpr are minimised.



5. Ensure the stamp extension, followed by the correct size stamp is in place. Replace with the correct size stamp if required.







Ortus Academy Ortus Academy is a trading name of Ortus Technology Limited. Company Registration 07554900

Academy_corpuls cpr Quick Guide_Scoopboard_Pause on Battery Exchange_SWV1.3_A046_v1

This document has been developed to provide users with an overview for safe device operation in accordance with its function and intended use and does not replace the user manual. All persons dealing with use, maintenance and troubleshooting must read and implement the user manual. Illustrations may not reflect that displayed on your device. Subject to technical modifications, mistakes, and printing errors.




Adjusting & Starting the cpr arm

 Remove the cpr arm from the bag and power on, review the therapy settings on the display screen and adjust if necessary.



2. With the arm facing away from the patient's chest, hold the cpr arm upright and align the bayonet fitting with the socket on the Scoopboard and click into position.



3. Release the locking lever and position so the stamp is in the middle of the lower part of the sternum, with the stamp touching the patient's chest.








 Optimum stamp positioning is reflected by the start / stop button LED illuminating green.

If the amber LED illuminates and the stamp is in visible contact with the chest, continue with the therapy.

If the red lamp is illuminated, raise the cpr arm until the green or amber LED illuminates and the stamp is visibly on the chest.



 Close the locking lever by slapping it with the palm of your open hand and then press the green or amber LED start / stop button.

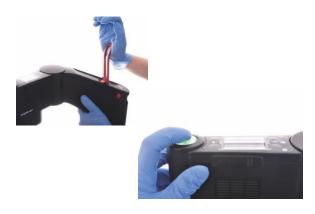

6. Mark the stamp position on the patient's sternum and review during rhythm checks.



Power Management

The remaining battery power can be reviewed by pressing the button below the battery LEDs.


If the battery is near depleted either:

1. Press the start / stop button to pause the OR 2. Plug the cpr arm into external power. therapy, remove the depleted battery by pressing the two red buttons and replace with a fully charged battery. Press the start / stop button to restart the therapy.




Adjusting Settings

Use the soft keys to adjust the therapy settings, if required.

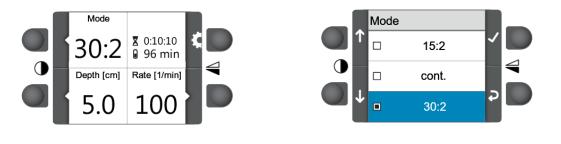


Alarm Management

Audible alerts via the loudspeaker and visual alarm notifications via the LED of the stop / start button and the display screen, are provided as High priority (red), Medium priority (yellow) and Low priority (cyan). The highest priority alarm will always be displayed.

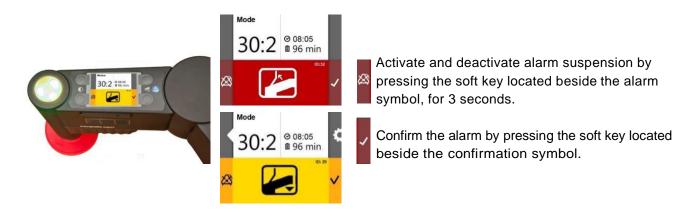



Ortus Academy Ortus Academy is a trading name of Ortus Technology Limited. Company Registration 07554900







Academy_corpuls cpr Quick Guide_Scoopboard_SWV1.3_A042_v1

This document has been developed to provide users with an overview for safe device operation with its function and intended use and does not replace the user manual. All persons dealing with use, maintenance and troubleshooting must read and implement the user manual. Illustrations may not reflect that displayed on your device. Subject to technical modifications, mistakes, and printing errors.




Securing the Fixation Ring


The Fixation Ring can be used to secure the patient to the Scoopboard in readiness for extrication. The attachment straps must be fastened to the Scoopboard and are freely accessible.

The user is responsible for checking the correct placement of the Fixation Ring and the stamp position during therapy.



 Either pause the therapy or during a ventilation pause, position the Fixation Ring centrally on the thorax, with the fasteners facing upright and hold in position.

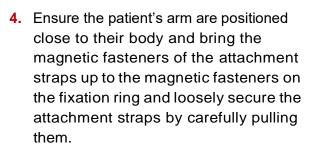





 Continue to hold the Fixation Ring in position and fully tighten the attachment straps by pulling them carefully and evenly in a diagonal direction on the patient's chest.



2. Additionally, the patient can be fully immobilised using the Patient Securing System.





Academy_corpuls cpr Quick Guide_Scoopboard_SWV1.3_A042_v1 This document has been developed to provide users with an overview for safe device operation in accordance

with its function and intended use and does not replace the user manual. All persons dealing with use, maintenance and troubleshooting must read and implement the user manual. Illustrations may not reflect that displayed on your device. Subject to technical modifications, mistakes, and printing errors.